

BS EN 60079-29-1:2016



BSI Standards Publication

Explosive atmospheres

Part 29-1: Gas detectors —
Performance requirements of
detectors for flammable gases

National foreword

This British Standard is the UK implementation of EN 60079-29-1:2016. It is derived from IEC 60079-29-1:2016. It supersedes BS EN 60079-29-1:2007 which is withdrawn.

The CENELEC common modifications have been implemented in the appropriate places in the text. The start and finish of each common modification is indicated in the text by tags \square and \square .

The UK participation in its preparation was entrusted by Technical Committee EXL/31, Equipment for explosive atmospheres, to Subcommittee EXL/31/1, Gas detectors.

A list of organizations represented on this subcommittee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2017.

Published by BSI Standards Limited 2017

ISBN 978 0 580 79858 0

ICS 13.320; 29.260.20

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 January 2017.

Amendments/corrigenda issued since publication

Date	Text affected
------	---------------

EUROPEAN STANDARD

EN 60079-29-1

NORME EUROPÉENNE

EUROPÄISCHE NORM

December 2016

ICS 29.260.20

Supersedes EN 60079-29-1:2007

English Version

Explosive atmospheres - Part 29-1: Gas detectors - Performance requirements of detectors for flammable gases
(IEC 60079-29-1:2016 , modified)

Atmosphères explosives - Partie 29-1: Détecteurs de gaz - Exigences d'aptitude à la fonction des détecteurs de gaz inflammables
(IEC 60079-29-1:2016 , modifiée)

Explosionsfähige Atmosphäre - Teil 29-1: Gasmessgeräte - Anforderungen an das Betriebsverhalten von Geräten für die Messung brennbarer Gase
(IEC 60079-29-1:2016 , modifiziert)

This European Standard was approved by CENELEC on 2016-09-19. CENELEC members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CENELEC member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CENELEC member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CENELEC members are the national electrotechnical committees of Austria, Belgium, Bulgaria, Croatia, Cyprus, the Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, the Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.



European Committee for Electrotechnical Standardization
Comité Européen de Normalisation Electrotechnique
Europäisches Komitee für Elektrotechnische Normung

CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels

Contents

Page

European foreword	3
Introduction	12
1 Scope	13
2 Normative references	14
3 Terms and definitions	14
4 General requirements	19
5 Test methods	26
Annexes	40
Annex ZA (normative) Normative references to international publications with their corresponding European publications	4
Annex ZZ (informative) Relationship between this European Standard and the essential requirements of Directive 2014/34/EU [2014 OJ L96] aimed to be covered	5
Bibliography	48

<http://www.china-gauges.com/>

European foreword

The text of document 31/1257/FDIS, future edition 2 of IEC 60079-29-1, prepared by IEC/TC 31 "Equipment for explosive atmospheres" was submitted to the IEC-CENELEC parallel vote and approved by CENELEC as EN 60079-29-1:2016.

A draft amendment, which covers common modifications to IEC 60079-29-1 (31/1257/FDIS), was prepared by SC 31-9 "Electrical apparatus for the detection and measurement of combustible gases to be used in industrial and commercial potentially explosive atmospheres", of CLC/TC 31 "Electrical apparatus for potentially explosive atmospheres" and approved by CENELEC.

The following dates are fixed:

- latest date by which the document has to be implemented at national level by publication of an identical national standard or by endorsement (dop) 2017-06-23
- latest date by which the national standards conflicting with the document have to be withdrawn (dow) 2019-12-23

This document supersedes EN 60079-29-1:2007.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CENELEC [and/or CEN] shall not be held responsible for identifying any or all such patent rights.

Clauses, subclauses, notes, tables, figures and annexes which are additional to those in IEC 60079-29-1:2016 are prefixed "Z".

This document has been prepared under a mandate given to CENELEC by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directive.

For the relationship with EU Directive see informative Annex ZZ, which is an integral part of this document.

Endorsement notice

The text of the International Standard IEC 60079-29-1:2016 was approved by CENELEC as a European Standard with agreed common modifications.

Annex ZA
(normative)

**Normative references to international publications
with their corresponding European publications**

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

NOTE 1 When an International Publication has been modified by common modifications, indicated by (mod), the relevant EN/HD applies.

NOTE 2 Up-to-date information on the latest versions of the European Standards listed in this annex is available here: www.cenelec.eu

<u>Publication</u>	<u>Year</u>	<u>Title</u>	<u>EN/HD</u>	<u>Year</u>
-	-	Electromagnetic compatibility - Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen	EN 50270	-
-	-	Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen - Requirements and tests for apparatus using software and/or digital technologies	EN 50271	-
IEC 60050-426	-	International Electrotechnical Vocabulary - Part 426: Equipment for explosive atmospheres	-	-
IEC 60068-2-6	-	Environmental testing - Part 2-6: Tests - Test Fc: Vibration (sinusoidal)	EN 60068-2-6	-
IEC 60079-0	-	Explosive atmospheres - Part 0: Equipment - General requirements	EN 60079-0	-
IEC 60079-20-1	-	Explosive atmospheres - Part 20-1: Material characteristics for gas and vapour classification - Test methods and data	EN 60079-20-1	-

Annex ZZ
(informative)

Relationship between this European Standard and the essential requirements of Directive 2014/34/EU [2014 OJ L96] aimed to be covered

This European Standard has been prepared under a Commission's standardization request [Full reference to the request "M/xxx" ¹⁾ to provide one voluntary means of conforming to essential requirements of *Directive 2014/34/EU of the European Parliament and of the Council of 26 February 2014 on the harmonisation of the laws of the Member States relating to equipment and protective systems intended for use in potentially explosive atmospheres* [2014 OJ L96].

Once this standard is cited in the Official Journal of the European Union under that Directive, compliance with the normative clauses of this standard given in Table ZZ.1 confers, within the limits of the scope of this standard, a presumption of conformity with the corresponding essential requirements of that Directive, and associated EFTA regulations.

Table ZZ.1 – Correspondence between this European Standard and Annex II of Directive 2014/34/EU [2014 OJ L96]

Essential Requirements of Directive 2014/34/EU	Clause(s) / sub-clause(s) of this EN	Remarks / Notes
1.5.5 - 1.5.7	whole standard except 4.2.9 and 5.4.23	
1.5.8	4.2.9, 5.4.23	

WARNING 1 — Presumption of conformity stays valid only as long as a reference to this European standard is maintained in the list published in the Official Journal of the European Union. Users of this standard should consult frequently the latest list published in the Official Journal of the European Union.

WARNING 2 — Other Union legislation may be applicable to the product(s) falling within the scope of this standard.

¹⁾ Mandate not yet available.

CONTENTS

FOREWORD.....	8
INTRODUCTION	2
1 Scope	13
2 Normative references	14
3 Terms and definitions	14
4 General requirements	19
4.1 Overview	19
4.1.1 Manufacturer claims	19
4.1.2 Equipment ratings	20
4.2 Construction	20
4.2.1 General	20
4.2.2 Indicating devices	20
4.2.3 Alarm signals	22
4.2.4 Fault signals	22
4.2.5 Adjustments	23
4.2.6 Battery-powered equipment	23
4.2.7 Gas detection transmitter for use with separate gas detection control units	23
4.2.8 Separate gas detection control units for use with gas detection transmitter(s)	23
4.2.9 Apparatus using software and/or digital technologies	24
4.3 Marking	24
4.4 Instruction manual	24
5 Test methods.....	26
5.1 Overview	26
5.2 General requirements for tests	26
5.2.1 General	26
5.2.2 Samples and sequence of tests	26
5.2.3 Preparation of equipment before testing	27
5.2.4 Mask for calibration and tests	28
5.3 Normal conditions for test	28
5.3.1 General	28
5.3.2 Test gas(es)	28
5.3.3 Standard test gas	28
5.3.4 Flow rate for test gases	29
5.3.5 Voltage	29
5.3.6 Temperature	29
5.3.7 Pressure	29
5.3.8 Humidity	29
5.3.9 Acclimation time	29
5.3.10 Orientation	29
5.3.11 Communications options	30
5.3.12 Gas detection equipment as part of systems	30

5.4	Test methods	30
5.4.1	General	30
5.4.2	Unpowered storage	30
5.4.3	Calibration and adjustment	31
5.4.4	Stability	31
5.4.5	Alarm set point(s)	32
5.4.6	Temperature	33
5.4.7	Pressure	33
5.4.8	Humidity of test gas	33
5.4.9	Air velocity	34
5.4.10	Flow rate for aspirated equipment	34
5.4.11	Orientation	34
5.4.12	Vibration	35
5.4.13	Drop test for portable and transportable equipment	35
5.4.14	Warm-up time	36
5.4.15	Time of response	36
5.4.16	High gas concentration operation above the measuring range	36
5.4.17	Battery capacity	37
5.4.18	Power supply variations	37
5.4.19	Addition of sampling probe	38
5.4.20	Other gases and poisons	38
5.4.21	Electromagnetic compatibility	38
5.4.22	Field calibration kit	38
5.4.23	Verification of software and digital components	39
Annex A	(normative) Performance requirements	40
Annex B	(informative) Determination of time of response	46
B.1	Aspirated equipment	46
B.1.1	Test rig	46
B.1.2	Equipment without internal pump	46
B.1.3	Equipment with internal pump	46
B.2	Equipment that samples by diffusion	47
B.2.1	Calibration mask method	47
B.2.2	Diffusion or flow methods	47
Bibliography	48
Figure 1	– Warm-up time in clean air (typical)	19
Figure 2	– Warm-up time in standard test gas (typical)	19
Figure B.1	– Schematic example of test rig for use with aspirated equipment	47
Table A.1	– Performance requirements (1 of 6)	40

INTERNATIONAL ELECTROTECHNICAL COMMISSION

EXPLOSIVE ATMOSPHERES –

Part 29-1: Gas detectors – Performance requirements of detectors for flammable gases

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (and National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publications for Flammable Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 60079-29-1 has been prepared by IEC technical committee 31: Equipment for explosive atmospheres.

This second edition of IEC 60079-29-1 cancels and replaces the first edition of IEC 60079-29-1:2007 series and constitutes a technical revision.

Significant technical changes between IEC 60079-29-1, Edition 1 (2007), and IEC 60079-29-1, Edition 2 (2016), is as listed below:

Significant changes with respect to IEC 60079-29-1:2007

Changes	Clause	Type		
		Minor and editorial changes	Extension	Major technical changes
Measuring range up to 20 %LEL (Modified requirements)	All		X	
Definitions (Additional clarifications)	3	X		
Manufacturer's claims (special applications requirements)	4.1.1			
General construction (Malfunction effects on safety related function)	4.2.1			C1
General indicating devices (portable equipment with visual and audible indication)	4.2.2.1			C2
Suppression of indication and measured values below zero (functional limits)	4.2.2.5			C3
Fault signals (Fault indication below minimum voltage limit, sensor disconnection and zero drift condition)	4.2.4			C4
Adjustments (Zero and sensitivity adjustments)	4.2.5			C5
Marking (Portable equipment protective case)	4.3		X	
Instruction Manual (Additions and clarifications)	4.4			C6
Samples and sequence of tests (Optical filter special sensitivity limits, and modification considerations)	5.2.2		X	
Preparation of equipment before testing (separate gas detection control units)	5.2.3	X		
Test gas (methane, and propane or butane for general purpose gas detector)	5.3.2			C7
General test methods (selectable range and wiring worst case conditions)	5.4.1		X	
Calibration curve (fixed volume fractions)	5.4.3.2			C8
Response to different gases (semiconductor and catalytic high gas concentration exposure)	5.4.3.3			C9
Stability (duration of test method)	5.4.4		X	
Alarm set point(s) (alarm set point test method)	5.4.5	X		
Temperature (portable) (temperature range and stabilization period)	5.4.6			C10
Temperature (all other equipment) (temperature range and stabilization period)	5.4.6		X	
Pressure (tolerance on pressure measurement)	5.4.7	X		
Humidity of test gas (test method clarification)	5.4.8	X		
Air velocity (test method clarification)	5.4.9	X		
Flow rate for aspirated equipment (test method clarification)	5.4.10	X		
Vibration (test method clarification)	5.4.12	X		

Changes	Clause	Type		
		Minor and editorial changes	Extension	Major technical changes
Drop test for portable and transportable equipment (Automatic re-starting or shut-down requirement clarification)	5.4.13	X		
Warm-up time (user prompt requirement)	5.4.14			C11
High gas concentration operation above the measuring range (test method and requirement clarification)	5.4.16			
Battery capacity (test method clarification)	5.4.17	X		
Power supply variation (minimum supply voltage fault limit)	5.4.18			C12
Poisons (applicable only to Group I apparatus with catalytic or semiconductor sensors) (test method clarification)	5.4.20.2	X		
Electromagnetic compatibility (test methods and requirements)	5.4.21			C13
Field calibration kit (test method clarification)	5.4.22	X		
Software function (supporting documentation)	5.4.23		X	
Determination of time of response (test method clarification)	Annex B		X	

NOTE 1 The technical changes referred to include the significance of technical changes in the revised IEC Standard, but they do not form an exhaustive list of all modifications from the previous version. More guidance may be found by referring to the Redline Version of the standard.

Explanations:

A) Definitions

Minor and editorial changes

Clarification decrease of technical requirements minor technical change editorial corrections.

These are changes which modify requirements in an editorial or a minor technical way. They include changes of the wording to clarify technical requirements without any technical change, or a reduction in level of existing requirement.

Extension

Addition of technical options

These are changes which add new or modify existing technical requirements, in a way that new options are given, but without increasing requirements for equipment that was fully compliant with the previous standard. Therefore, these will not have to be considered for products in conformity with the preceding edition.

Major technical changes

Addition of technical requirements increase of technical requirements.

These are changes to technical requirements (addition, increase of the level or removal) made in a way that a product conforming to the preceding edition will not always be able to fulfil the requirements given in the later edition. These changes have to be considered for products conforming to the preceding edition. For these changes additional information is provided in B) below.

NOTE 2 These changes represent current technological knowledge. However, these changes should not normally have an influence on equipment already placed on the market.

B) Information about the background of 'Major technical changes'

- C1 Addition of malfunction effects not adversely affecting the safety related function (4.2.1).
- C2 Addition of visual and audible indication for portable equipment (4.2.2.1).
- C3 Addition of functional limits for suppression of indication and for measured values below zero (4.2.2.5).
- C4 Addition of requirements for fault indication below minimum voltage limit, sensor disconnection and zero drift condition (4.2.4).
- C5 Addition of requirements for zero and sensitivity adjustments (4.2.5).
- C6 Addition and clarification requirements for inclusion within the instruction manual (4.4).
- C7 Addition of methane and propane or butane as required test gases for general purpose gas detector (5.3.2).
- C8 Specification of fixed volume fractions which are expressed as a percentage of the measuring range (5.4.3.2).
- C9 Addition of requirement for semiconductor and catalytic sensors to be exposed to high gas concentration on response to different gases (5.4.3.3).
- C10 Addition of temperature range and stabilization period (5.4.6).
- C11 Addition of requirement where equipment prompts the user (5.4.14).
- C12 Addition of requirement for output functionality above the minimum supply voltage fault limit (5.4.18).
- C13 Addition of test methods and requirements for electromagnetic compatibility tests (5.4.21).

The text of this standard is based on the following documents:

FDIS	Report on voting
31/1257/FDIS	31/1266/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of the IEC 60079 series, under the general title *Explosive atmospheres*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

A bilingual version of this publication may be issued at a later date.

INTRODUCTION

This part of IEC EN 60079-29 IEC specifies general requirements for construction, testing and performance, and describes the test methods that apply to portable, transportable and fixed equipment for the detection and measurement of flammable gas or vapour concentrations with air.

Guidance for the selection, installation, use and maintenance of gas detecting equipment is set out in IEC EN 60079-29-2 IEC: *Explosive atmospheres – Part 29-2: Gas detectors – Selection, installation, use and maintenance of detectors for flammable gases and oxygen.*

Guidance for functional safety of fixed gas detection systems is set out in IEC EN 60079-29-3 IEC: *Explosive atmospheres – Part 29-3: Gas detectors – Guidance on functional safety of fixed gas detection systems.*

General requirements for construction, testing and performance of open path detectors for flammable gases are set out in IEC EN 60079-29-4 IEC: *Explosive atmospheres – Part 29-4: Gas detectors – Performance requirements of open path detectors for flammable gases.*

EXPLOSIVE ATMOSPHERES –

Part 29-1: Gas detectors – Performance requirements of detectors for flammable gases

1 Scope

This part of IEC EN 60079-29 IEC specifies general requirements for construction, testing and performance, and describes the test methods that apply to portable, transportable and fixed equipment for the detection and measurement of flammable gas or vapour concentrations with air. The equipment, or parts thereof, is intended for use in explosive atmospheres and in mines susceptible to fire and explosion.

This part of IEC EN 60079-29 IEC is applicable to flammable gas detection equipment with a measuring range up to any volume fraction as declared by the manufacturer, and which is intended to provide an indication, alarm or other output function; the purpose of which is to indicate a potential explosion hazard and in some cases, to initiate automatic or manual protective action(s).

For the purposes of this part of IEC EN 60079-29 IEC, the term “indicating up to a volume fraction of X % or X %LFL” includes equipment with an upper limit of the measuring range equal to or less than X % or X %LFL.

This part of IEC EN 60079-29 IEC is applicable to equipment, including the integral sampling systems of aspirated equipment, intended to be used for commercial, industrial and non-residential safety applications.

This part of IEC EN 60079-29 IEC does not apply to external sampling systems, or to equipment of laboratory or scientific type, or to equipment used only for process monitoring and/or control purposes. It also does not apply to open path (line of sight) detectors which are within the scope of IEC EN 60079-29-4 IEC. Only equipment with very short optical paths intended for use where the concentration is uniform over the optical path are within the scope of this standard.

For equipment used for sensing the presence of multiple gases, this part of IEC EN 60079-29 IEC applies only to the detection of flammable gas or vapour.

This part of IEC EN 60079-29 IEC supplements and modifies the general requirements of IEC EN 60079-0 IEC. Where a requirement of this standard conflicts with a requirement of IEC EN 60079-0 IEC, the requirement of IEC EN 60079-29-1 IEC takes precedence.

IEC Text deleted IEC

NOTE IEC 1 IEC All equipment calibrated on specific gases or vapours can not be expected to correctly indicate on other gases or vapours.

For the purposes of this standard, the terms “lower flammable limit (LFL)” and “lower explosive limit (LEL)” are deemed to be synonymous, and likewise the terms “upper flammable limit (UFL)” and “upper explosive limit (UEL)” are deemed to be synonymous. For ease of reference, the two abbreviations LFL and UFL may be used hereinafter to denote these two sets of terms. It should be recognized that particular authorities having jurisdiction may have overriding requirements that dictate the use of one of these sets of terms and not the other.

NOTE IEC 2 IEC Indication of concentration in %(v/v) or vol ppm can also be available for equipment which measures up to 100 %LFL or 20 %LFL. In that case, units of measurement might need to be selected in agreement with the manufacturer when verifying the performance requirements of Annex A.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

☐ EN 50270, *Electromagnetic compatibility – Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen*

EN 50271, *Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen – Requirements and tests for apparatus using software and/or digital technologies* ☐

☐ EN 60079-0 ☐, *Explosive atmospheres – Part 0: Equipment – General requirements*

☐ EN 60068-2-6 ☐, *Environmental testing – Part 2-6: Tests – Test Fc: Vibration (sinusoidal)*

☐ EN 60079-20-1 ☐, *Explosive atmospheres – Part 20-1: Material characteristics for gas and vapour classification – Test methods and data*

IEC 60050-426, *International Electrotechnical Vocabulary – Part 426: Equipment for explosive atmospheres*

☐ *Text deleted* ☐

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ☐ EN 60079-0 ☐ and the following apply. Additional definitions applicable to explosive atmospheres can be found in IEC 60050-426.

3.1 gas properties

3.1.1 ambient air

normal atmosphere surrounding the equipment

3.1.2 clean air

air that is free of gases or vapours which the sensor is sensitive to or which influence the performance of the sensor

3.1.3 flammable gas

gas or vapour which, when mixed with air in a certain proportion, will form an explosive atmosphere

Note 1 to entry: For the purposes of this part of ☐ EN 60079-29 ☐, the term “flammable gas” includes flammable vapours.

Note 2 to entry: For the purposes of this part of ☐ EN 60079-29 ☐, the terms “combustible gas” and “flammable gas” are equivalent.

3.1.4 lower flammable limit

LFL

concentration of flammable gas or vapour in air, below which an explosive gas atmosphere does not form

☐ Note 1 to entry: This is also known as lower explosive limit (LEL). ☐

Note 2 to entry: The concentration may be expressed as either a volume fraction or a mass per unit volume.

3.1.5 poisons

<for sensing elements> substances that lead to temporary or permanent change of performance, particularly loss of sensitivity of the sensing element

3.1.6 upper flammable limit

UFL

concentration of of flammable gas or vapour in air, above which an explosive gas atmosphere does not form

☐ Note 1 to entry: This is also known as upper explosive limit (UEL). ☐

Note 2 to entry: The concentration may be expressed as either a volume fraction or a mass per unit volume.

3.1.7 volume fraction

v/v

quotient of the volume of a specified component and the sum of the volumes of all components of a gas mixture before mixing, all volumes referring to the pressure and the temperature of the gas mixture

Note 1 to entry: The volume fraction and volume concentration take the same value if, at the same state conditions, the sum of the component volumes before mixing and the volume of the mixture are equal. However, because the mixing of two or more gases at the same state conditions is usually accompanied by a slight contraction or, less frequently, a slight expansion, this is not generally the case.

3.1.8 zero gas

gas recommended by the manufacturer, which is free of flammable gases and interfering and contaminating substances, the purpose of which is calibration/adjustment of the equipment zero

3.1.9 standard test gas

test gas with a composition specified for each item of equipment and gas and/or vapour to be used for all tests unless otherwise stated

3.2 types of equipment

3.2.1 alarm-only equipment

equipment with an alarm but not having an indication of measured value

3.2.2 aspirated equipment

equipment that samples the gas by drawing it to the gas sensor

Note 1 to entry: A hand operated or electric pump is often used to draw gas to the sensor.

3.2.3 automatically aspirated equipment

aspirated equipment with an integral pump or separate pump, which is connected directly to the equipment

3.2.4

continuous duty equipment

equipment that is powered for long periods of time, but may have either continuous or intermittent sensing

Note 1 to entry: For this edition of the standard, all equipment is regarded as continuous duty.

3.2.5

diffusion equipment

equipment in which the transfer of gas from the atmosphere to the sensor takes place without aspirated flow

3.2.6

equipment, fixed

equipment fastened to a support, or otherwise secured in a specific location when energized

3.2.7

Group I equipment

equipment for mines susceptible to firedamp

3.2.8

Group II equipment

equipment for places with an explosive gas atmosphere, other than mines susceptible to firedamp

3.2.9

equipment, portable

equipment intended to be carried by a person during operation

Note 1 to entry: A portable equipment is battery powered and includes, but is not limited to

- a) a hand-held equipment, typically less than 1 kg, which requires use of only one hand to operate,
- b) personal monitors, similar in size and mass to the hand-held equipment, that are continuously operating (but not necessarily continuously sensing) while they are attached to the user, and
- c) larger equipment that can be operated by the user while it is carried either by hand, by a shoulder strap or carrying harness and which may or may not have a hand directed probe.

3.2.10

equipment, transportable

equipment not intended to be carried by a person during operation, nor intended for fixed installation

3.2.11

gas detection transmitter

fixed gas detection equipment that provide a conditioned electronic signal or output indication to a generally accepted industry standard (such as 4 to 20 mA), intended to be utilized with separate gas detection control units or signal processing data acquisition, central monitoring and similar systems, which typically process information from various locations and sources including, but not limited to gas detection equipment

3.2.12

gas detection control unit

equipment intended to provide display indication, alarm functions, output contacts and/or alarm signal outputs or any combinations when operated with remote sensor(s)

3.2.13

separate gas detection control unit

equipment intended to provide display indication, alarm functions, output contacts or alarm signal outputs or any combination when operated with gas detection transmitter(s)

3.2.14

equipment with integral sensor(s)

equipment that provides display indication, alarm functions, output contacts and/or alarm signal outputs using a sensor which is within or directly mounted to the equipment housing.

3.2.15

accessory

component which can be fitted to the equipment for special purpose

EXAMPLE External gas pump, sampling probe, hoses, collecting cone, weather protection device

3.3

sensors

3.3.1

sensing element

part of the sensor which is sensitive to the gas/vapour to be measured

3.3.2

sensor

assembly in which the sensing element is housed and that may also contain associated circuit components

3.3.3

integral sensor

sensor which is within or directly mounted to the equipment housing

3.3.4

remote sensor

sensor that is separated from the equipment body and is connected to a gas detection control unit or to a gas detection transmitter.

3.4

supply of gas to equipment

3.4.1

sample line

means by which the gas being sampled is conveyed to the sensor

Note 1 to entry: Accessories such as filter or water trap are often included in the sample line.

3.4.2

sampling probe

separate accessory sample line which is optionally attached to the equipment

Note 1 to entry: It is usually short (e.g. of the order of 1 m) and rigid, although it can be telescopic. In some cases it is connected by a flexible tube to the equipment.

3.4.3

field calibration kit

means of presenting test gas to the equipment for the purpose of calibrating/adjusting or verifying the operation of the equipment

Note 1 to entry: The field calibration kit can be used for verifying the operation of the alarms if the concentration of the test gas is above the alarm set-point.

Note 2 to entry: A mask for calibration and test (see 3.4.4) is an example of a field calibration kit.

3.4.4

mask for calibration and test

device that can be attached to the equipment to present a test gas to the sensor in a reproducible manner

3.5 signals and alarms

3.5.1 alarm set point

setting of the equipment at which the measured concentration will cause the equipment to initiate an indication, alarm or other output function

3.5.2 latching alarm

alarm that, once activated, requires deliberate action to be deactivated

3.5.3 fault signal

audible, visible or other type of output, different from the alarm signal, permitting, directly or indirectly, a warning or indication that the equipment is not working satisfactorily

3.5.4 special state

any state of the equipment other than those in which monitoring of gas concentration and/or alarming is the intent

Note 1 to entry: Special state includes warm-up, calibration mode or fault condition.

3.6 times

3.6.1 drift

variation in the equipment indication over time at any fixed gas volume fraction (including clean air) under constant ambient conditions

3.6.2 final indication

indication given by the equipment after stabilization

3.6.3 stabilization

state when three successive readings of an equipment at a constant gas volume fraction, taken at 2 min intervals or twice the respective $t(90)$, whichever is less, indicates no changes greater than ± 1 % of the measuring range

3.6.4 time of response

$t(x)$

time interval, with the equipment in a warmed-up condition, between the time when an instantaneous change between clean air and the standard test gas, or vice versa, is produced at the equipment inlet, and the time when the response reaches a stated percentage (x) of the stabilized signal on the standard test gas

3.6.5 warm-up time

time interval, with the equipment in a stated atmosphere, between the time when the equipment is switched on and the time when the indication reaches and remains within the stated tolerances

Note 1 to entry: See Figure 1 and Figure 2.

<http://www.china-gauges.com/>

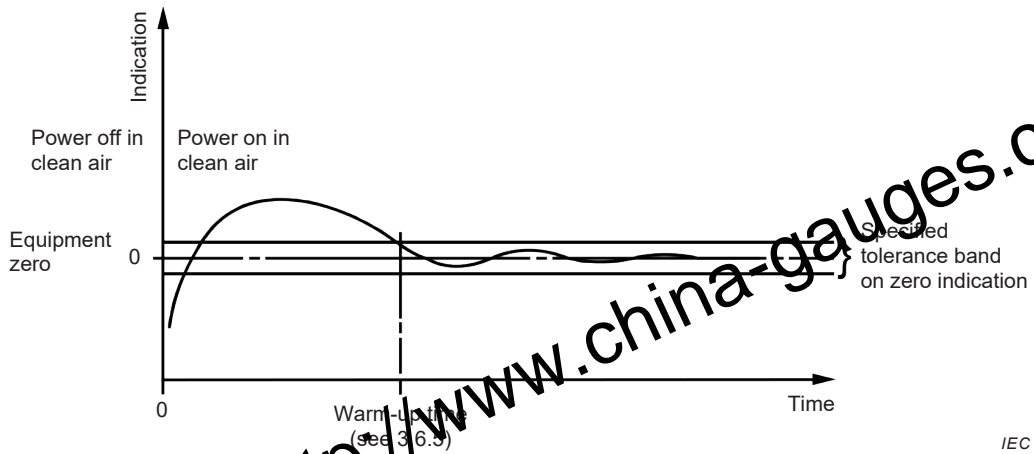


Figure 1 – Warm-up time in clean air (typical)

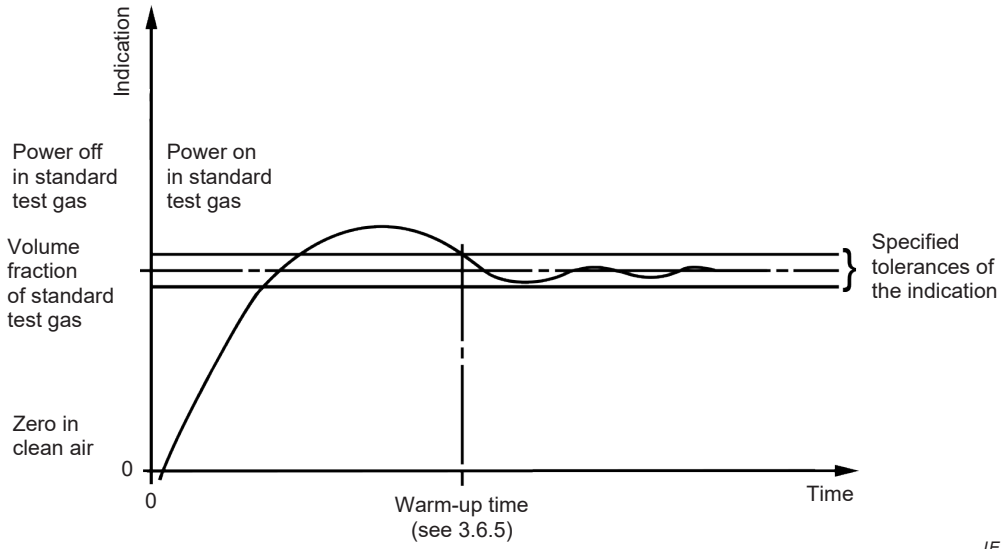


Figure 2 – Warm-up time in standard test gas (typical)

3.7 miscellaneous

3.7.1 special tool

tool required to gain access to, or to adjust the equipment controls

Note 1 to entry: The design of the tool is intended to discourage unauthorised interference with the equipment.

4 General requirements

4.1 Overview

4.1.1 Manufacturer claims

The equipment shall conform to the requirements of this part of [C] EN 60079-29 [C] and Annex A criteria.

Where an equipment manufacturer makes any claims in the instruction manual regarding any special features of construction or superior performance that exceed these minimum requirements, all such claims shall be verified and the test procedures shall be carried out as stated in each clause and shall be extended or supplemented, where necessary, to verify the claimed performance.

When verifying a manufacturer's claimed performance or special features of construction, the minimum requirements of the standard shall be met and the manufacturer's claimed performance shall be verified. Any additional tests shall be agreed upon by the manufacturer and test laboratory and identified and described in the test report.

EXAMPLE When a manufacturer claims a sensor accuracy over a defined temperature range of $-50\text{ }^{\circ}\text{C}$ to $+55\text{ }^{\circ}\text{C}$ at $\pm 15\%$ LFL (assuming a measuring range of 0 to 100 % LFL), the sensor must meet the manufacturer's claim from $-50\text{ }^{\circ}\text{C}$ to $-20\text{ }^{\circ}\text{C}$ and meet the specified requirements of 5.4.6 for the temperature range of $-20\text{ }^{\circ}\text{C}$ to $+55\text{ }^{\circ}\text{C}$.

There may be applications where equipment with special features are needed. One example may be a gas detector intended to be used in coal mines with a measuring range up to 10 % (v/v) methane but with the accuracy requirements of 5 % (v/v) methane equipment. In such a case it shall be tested like 5 % (v/v) methane equipment.

4.1.2 Equipment ratings

Electrical assemblies and components shall conform to the construction and test requirements of 4.2 and Clause 5, where applicable. In addition, parts of the flammable gas detection equipment intended for use in hazardous areas shall conform to the Type(s) of Protection as specified \square in the appropriate regulations for explosion protection \square .

The ambient temperature and pressure ranges of equipment conforming to this standard shall not exceed the ambient temperature and pressure ranges of the Type(s) of Protection.

4.2 Construction

4.2.1 General

Gas detection equipment or parts thereof (e.g. remote sensors) specifically intended for use in the presence of corrosive vapours or gases, or which may produce corrosive by-products as a result of the detection process (e.g. catalytic oxidation or other chemical process) shall be constructed of materials known to be resistant to corrosion by such substances.

All equipment shall be constructed to facilitate regular accuracy checks.

All materials and components used in the construction of the equipment shall be used within the manufacturer's ratings or limitations, unless otherwise specified by appropriate safety standards.

Any malfunction of outputs from the gas detection equipment not relevant to safety or health shall not adversely affect the functions of the equipment related to safety.

EXAMPLE Equipment with 4-20 mA and HART communication where only the 4-20 mA communication is defined in the instruction manual as related to safety. The loss of HART communication is not related to safety.

4.2.2 Indicating devices

4.2.2.1 General

Readily distinguishable indications shall be provided to show that the equipment is energized, in alarm and in special states.

Portable equipment shall provide visual and audible indications for both fault and alarms.

If audible indications are provided for transportable or fixed equipment, alarms shall be indicated as a minimum.

All methods of indication of the measured value shall present the same value within the resolution of each indicator.

The indications related to gas detection transmitters and remote sensors for fixed equipment may be shown only at the (separate) gas detection control unit.

4.2.2.2 Resolution

For alarm-only equipment or equipment where the resolution of the read-out device is inadequate to demonstrate compliance with this standard, the manufacturer shall identify suitable points for connecting indicating or recording devices for the purpose of testing the compliance of the equipment with this standard. The indication on the readout device shall not contradict the results obtained by additional indicating or recording devices.

4.2.2.3 Measuring range

Any over-range measurements shall be clearly indicated as such.

4.2.2.4 Selectable range

If the equipment has more than one measuring range, the range selected shall be clearly identified.

4.2.2.5 Suppression of indication and measured values below zero

It shall be possible to configure the equipment such that in measuring mode any kind of suppression of the measured value is permanently disabled. In calibration mode any kind of suppression of the measured value shall be automatically disabled.

Measured values within the measuring range shall be indicated.

Measured values below 5 % of the measuring range (values below zero included) shall be indicated as:

- a) zero,
- b) another indication that the measured value is below 5 % of the measuring range or
- c) the measured value.

Equipment with a measuring range up to 20 % LFL shall indicate measured values below -10 % of the measuring range or shall provide a fault signal. The equipment shall provide a fault signal at measured values below -20 % of the measuring range at the latest.

All equipment with measuring ranges greater than 20 % LFL shall provide a fault signal at measured values below -10 % of the measuring range at the latest. Portable and transportable equipment shall indicate measured values below -5 % of the measuring range or shall provide a fault signal.

Any suppression of indication shall be explained in the manual (see 4.4 d)).

4.2.2.6 Indicator light

If only one indicator light is provided for signalling alarms, special states and other indications, it shall be coloured red. If separate indicator lights are used or if a multi-coloured indicator light is provided, the colours shall be used in the following order of priority ((a) being highest priority):

- a) alarms indicating the presence of a gas concentration beyond an alarm set point shall be coloured RED;
- b) equipment special state indicators shall be coloured YELLOW;
- c) power supply indicators shall be coloured GREEN.

If there is more than one indicator light of the same colour with different functions, the lights shall be labelled to show their functions. Text, marks, and icons on a screen display describing the indicator lights are permissible in place of printed labels.

4.2.3 Alarm signals

4.2.3.1 General

Alarm devices shall not be adjustable to operate outside the measuring range.

If alarm devices, output contacts or alarm signal outputs are provided as part of continuous duty gas detection equipment and are intended to operate when a potentially hazardous gas concentration is detected, they shall be of a latching type requiring a deliberate manual action to reset. If two or more alarm set points are provided, the lower may be non-latching – based on user preference. Alarms shall remain in operation while the alarm condition is still present, although audible alarms may be silenced if this audible alarm is not the only alarm.

If it is possible to deactivate alarm devices, output contacts or alarm signal outputs, e.g. for calibration purposes, this deactivation shall be indicated by a signal. For fixed equipment, this shall include a contact or other transmittable output signal. However, the output signal or contacts are not required if the alarms are automatically re-enabled within 15 min.

4.2.3.2 Group I portable equipment indicating up to 5 % (v/v)

Alarm devices shall not be adjustable above 3 % (v/v). An additional over-range alarm, which indicates when full scale has been exceeded, may be provided.

4.2.3.3 Group II portable equipment indicating up to 100 % LFL

Alarm devices shall not be adjustable above 60 % LFL. An additional over-range alarm, which indicates when full scale has been exceeded, may be provided.

4.2.4 Fault signals

Fixed and externally powered transportable equipment shall provide a fault signal in the event of failure of power to the equipment.

Externally powered equipment shall provide a fault signal when the power supply falls below the manufacturer's specified minimum supply voltage fault limit.

A short-circuit or open-circuit in connections to any remote sensor or gas detection transmitter shall be indicated by a fault signal.

Under the above conditions the equipment may also indicate alarm.

Measured values below zero (e.g. caused by drift) shall be indicated by a fault signal in accordance with the conditions of 4.2.2.5.

For equipment where the sensor can be disconnected without opening the housing, the equipment shall provide a fault signal in the event of a disconnection of the sensor.

Automatically aspirated equipment shall be provided with an integral flow-indicating device that produces a fault signal in the event of low flow.

4.2.5 Adjustments

All adjustment devices shall be designed so as to discourage unauthorized or inadvertent interference with the equipment. Examples include procedural devices, in the case of a keyboard instrument, or mechanical devices such as a cover requiring the use of a special tool.

Fixed explosion-protected equipment housed in explosion-protected enclosures shall be designed so that, if any facilities for adjustment are necessary for recalibration and for resetting or like functions, these facilities shall be externally accessible. The means for making adjustments shall not degrade the explosion protection of the equipment.

The adjustments of the zero and sensitivity shall be designed so that:

a) adjustment of one will not affect the other;

or

b) it shall not be possible to adjust only one and the sequence of adjustments shall ensure that the affected one is adjusted second.

The equipment shall not perform an automatic zero adjustment during start-up. If equipment prompts the user for zero adjustment during start-up and the user makes no selection, equipment shall continue to start-up without zero adjustment, after a delay of no more than 15 s.

4.2.6 Battery-powered equipment

Equipment powered with integral batteries shall be provided with an indication of low battery condition, and the purpose of this indication shall be explained in the manual (see 4.4 j)).

4.2.7 Gas detection transmitter for use with separate gas detection control units

A specification shall be supplied with the equipment that describes the relationship the gas concentration (detected by the equipment) has with the corresponding output signal or indication (transfer function). Such specification shall be detailed to the extent that the accuracy of this transfer function can be verified. As a minimum, the manufacturer shall provide data showing the relationship between the output signal and the gas concentrations corresponding to 0 %, 10 %, 30 %, 50 %, 70 %, 90 % and 100 % of full-scale output indication. Full-scale output and status signals (e.g. fault, inhibit) shall also be specified by the manufacturer.

Where necessary, equipment shall be provided by the manufacturer to interpret the output signal or indication, which will enable the accuracy of the transfer function to be verified.

4.2.8 Separate gas detection control units for use with gas detection transmitter(s)

A specification shall be supplied with the equipment that describes the relationship the input signal has with the calculated gas concentration (transfer function). Such specification shall be detailed to the extent that the accuracy of this transfer function can be verified. As a minimum, the manufacturer shall provide data showing the relationship between the input signal and the gas concentrations corresponding to 0 %, 10 %, 30 %, 50 %, 70 %, 90 % and 100 % of full-scale output indication. Required inputs for full-scale indication and status signals (e.g. fault, inhibit) shall also be specified by the manufacturer.

Where necessary, equipment shall be provided by the manufacturer to provide the input signals, which will enable the accuracy of the transfer function to be verified.

4.2.9 Apparatus using software and/or digital technologies

The equipment shall fulfil the requirements of EN 50271.

Software-controlled accessories shall be included where related to safety.

4.3 Marking

In addition to the applicable marking requirements of EN 60079-0, the equipment marking shall also include:

- a) EN 60079-29-1 (to represent conformance with this performance standard);
- b) year of construction (may be encoded within the serial number).

For portable equipment requiring the use of a protective case in normal operation, the required markings shall not be obscured or shall be reproduced on the protective case.

For small gas detection equipment, the EN 60079-29-1 marking may be placed within the manual.

4.4 Instruction manual

Each equipment shall be provided with an instruction manual that includes the following information as relevant:

- a) complete instructions, drawings and diagrams for safe and proper operation, installation and servicing of the equipment;
- b) operating instructions and calibration/adjustment procedures including ranges of concentration and humidity of the test gases as well as instructions for the use of the field calibration kit (see also 5.4.22);
- c) details for calibration and/or maintenance which shall include the following:
 - 1) recommendations for initial checking and calibration of the equipment on a routine basis including the maximum time interval between calibrations;
 - 2) for portable equipment the requirement and method for performing a functional check with gas before each day of use;
 - 3) recommendations for maintenance to be taken after the measuring range has been exceeded;
 - 4) the procedure to check reaction time when the calibration gas is applied;
 - 5) a recommendation to users to read the procedures described in EN 60079-29-2 for reference.
- d) details of operational limitations, performance claimed by the manufacturer and special features including, where applicable, the following:
 - 1) gases for which the equipment is suitable and the relative sensitivities including tolerances to these gases;
 - 2) information that describes the sensitivities to other gases to which the equipment is responsive;
 - 3) time of response $t(90)$ for the standard test gas(es), method of test (diffusion or flow), and $t(90)$ for other gases tested in accordance with this standard;
 - 4) temperature limits (explosion protection and performance);
 - 5) humidity limits;
 - 6) pressure limits (explosion protection and performance);
 - 7) supply voltage limits;
 - 8) maximum power consumption;

- 9) relevant characteristics and construction details of required interconnecting cables;
 - 10) for battery operated equipment, battery type(s) and operating time(s) until low battery condition under normal operating conditions;
 - 11) sample flow rate limits;
 - 12) warm-up time;
 - 13) test gas application time for calibration;
 - 14) nominal orientation and orientation limits (for fixed and transportable equipment);
 - 15) electro-magnetic compatibility (e.g. shielded cable, transient suppression, special enclosure);
 - 16) description of any suppression of, indication and method for its enablement/disablement;
 - 17) air velocity limits.
- e) details of storage and limitations for the equipment, replacement parts and accessories, including, where applicable, the following:
- 1) temperature;
 - 2) humidity;
 - 3) pressure;
 - 4) time.
- f) bases (source(s) and edition(s), such as [EN 60079-20-1](#)) used for converting test and calibration gas concentrations from % LFL to % volume fraction;
- g) information on the adverse effects of poisons and interfering gases or substances and oxygen-enriched or deficient atmospheres on the proper performance (and, in the case of oxygen-enriched atmospheres, on electrical safety) of the equipment;
- h) for aspirated equipment, indication of the minimum and maximum flow rates and pressure, tubing type, maximum length and size for proper operation;
- i) for aspirated equipment, instructions for ensuring that the sample lines are intact and that proper flow is established (see 4.2.4);
- j) specification and significance of each alarm (including over-range indication) and fault signal, the default setting of alarms, the duration of such alarms and signals (if time-limited or non-latching), and any provisions that may be made for silencing or resetting such alarms and signals, as applicable;
- k) details of any method for the determination of the possible sources of a malfunction and any corrective procedures (i.e. trouble-shooting procedures);
- l) a statement that alarm devices, outputs or contacts are of the non-latching types, where applicable (see 4.2.3.1);
- m) for battery-operated equipment, installation and maintenance instructions for the batteries;
- n) a recommended replacement parts list;
- o) where optional accessories (e.g. collecting cones, weather-protecting devices, field calibration kit) are supplied, a list of such accessories and their effects on the instrument characteristics (including response time and sensitivity), and means for their identification (e.g. part numbers). In addition, it shall be clearly described for each accessory whether it is included in the performance certificate. Consideration shall be given to the effects of the use of the accessory on the measurement of different gases (see d)1) and d)3));
- p) details of performance certification, if any (e.g. issuing organisation, date, ranges, gases, accessories, etc.), and marking, and any special conditions of use;
- q) if an ingress protection (IP) is claimed, such as [EN 60529](#), the following statement shall be included:
- 1) IP ratings do not imply that the equipment will detect gas during and after exposure to those conditions.

- 2) recommendations for determining appropriate calibration interval and maintenance requirements if exposed to those conditions representative of the IP rating;
- 3) recommended accessories to those conditions representative of the IP rating
- r) for gas detection transmitter or separate gas detection control units, specification of the transfer function, full scale input/output and all status signals (e.g. fault, inhibit) (see 4.2.7 and 4.2.8);
- s) for gas detection transmitter or separate gas detection control unit, information that the time of response of the entire system is determined by the time of response of all parts of equipment within the gas detection system;
- t) for gas detection control unit or separate gas detection control unit, the maximum delay time until special state is entered in case of transmission errors;
- u) any necessary instructions or information, where the special nature of the equipment (such as non-linear responses) requires additional instructions or special information that are alternative to, or in addition to, the requirements of 4.3 and 4.4 a) to r).

5 Test methods

5.1 Overview

The test methods and procedures described in 5.2 to 5.4 are intended as a basis for establishing whether the equipment conforms with the supplementary requirements for performance given in Annex A.

5.2 General requirements for tests

5.2.1 General

Where it is necessary to apply LFL and UFL values for the purposes of this standard, reference shall be made to [\[C\]](#) EN 60079-20-1 [\[C\]](#).

5.2.2 Samples and sequence of tests

5.2.2.1 General

For the purpose of type testing, all the tests shall be carried out on the same sample except for tests 5.4.4.3 to 5.4.4.6 in combination with 5.4.16 and for test 5.4.20, each of which may be conducted on separate samples.

5.2.2.2 Optical filter

For IR-sensors with optical filters, where relative sensitivities with tolerance less than 20 % of the stated value are specified within the instruction manual (see 4.4 d)1), the test 5.4.3.3 shall be conducted with two samples where the centre wavelength of the optical filters shall be at the minimum and maximum limits of the specification. One of these units may be used subsequently for 5.4.4.3 to 5.4.4.6, 5.4.16 and 5.4.20.

5.2.2.3 Sequence

The unpowered storage test (5.4.2) shall be conducted prior to all remaining tests. The vibration test (5.4.12) shall be performed after unpowered storage testing for pre-conditioning purposes.

All remaining tests shall be performed to a schedule agreed upon between the manufacturer and the test laboratory. However, the tests 5.4.4.3 to 5.4.4.6 and 5.4.16 shall always be conducted sequentially.

If the design of equipment, which has been tested previously to this standard, is modified then the test laboratory shall agree with the manufacturer which tests have to be repeated with the modified equipment. The decision and its justification shall be described in the test report.

In the case of modifications to the software or of electronic components which are part of the basic gas detection functionality (signal chain from sensor to output(s)) the following tests shall be re-performed as a minimum: calibration curve, alarm set point(s), time of response.

5.2.2.4 Gas detection transmitter(s)

Gas detection transmitter(s) shall be tested to the applicable requirements of 5.4.2 through 5.4.12 and 5.4.14 through 5.4.23 using the parameters of the transfer function.

5.2.2.5 Separate gas detection control units

Separate gas detection control units shall be tested to the applicable requirements of 5.4.2, 5.4.3, 5.4.5, 5.4.6, 5.4.12, 5.4.14 through 5.4.18, 5.4.21 and 5.4.23 using the parameters of the transfer function(s).

5.2.3 Preparation of equipment before testing

The equipment shall be prepared and mounted as near to typical use as possible, in accordance with the instruction manual, including all necessary interconnections, initial adjustments and initial calibrations. Adjustments may be made, where appropriate, at the beginning of each test in 5.4.2 to 5.4.23. During each test, no adjustment shall be made. Suppression of indications of the equipment under test shall be disabled.

Optional accessories to be included in the performance test shall be either attached or removed according to which condition will give the most unfavourable result for the test being conducted unless otherwise specified. The exact configuration of the equipment, including use of or removal of the optional accessories, shall be included in the test report.

EXAMPLE Weather protection is an example of an optional accessory.

In particular, the following points shall be noted:

a) All equipment having remote sensors:

- For the purpose of the tests in 5.4, where reference is made to exposure of the sensor to the test conditions, the entire remote sensor (including any or all normally attached protective mechanical parts) shall be exposed.
- For equipment having connection facilities for more than one remote sensor, only one remote sensor needs to be subjected to the tests. The replacement of all but one sensor by "dummy" impedances yielding the worst case load conditions for the test in question shall be permitted. The worst case load conditions shall be determined by the testing laboratory within the limits specified in the instruction manual (see 4.4 d)).
- For equipment having remote sensor(s), all tests shall be performed with resistances connected in the detector circuit to simulate the maximum line resistance specified by the manufacturer, except where minimum line resistance offers a more stringent test in the judgement of the test laboratory.

b) Separate gas detection control units:

The replacement of all transmitters by appropriate signal sources and worst case loads for the test in question shall be permitted. The worst case loads shall be determined by the test laboratory within the limits specified in the instruction manual (see 4.4 d)).

c) All equipment having integral sensors:

The entire equipment shall be exposed to the test conditions without removal of any normally attached parts, including any sampling probe for tests 5.4.10, 5.4.14 and 5.4.15 .

d) Alarm-only equipment:

For alarm-only equipment, readings shall be taken using an indicating or recording device connected to the test points described in 4.2.2.2.

5.2.4 Mask for calibration and tests

When a mask is used for calibration or for the injection of test gas into the sensor, the design and operation of the mask used by the testing laboratory – in particular the pressure and velocity inside the mask – shall not influence the response of the equipment or the results obtained.

The manufacturer may provide a suitable calibration mask together with details of pressure or flow for application of calibration gases with the equipment.

5.3 Normal conditions for test

5.3.1 General

The test conditions specified in 5.3.2 to 5.3.12 shall be used for all tests, unless otherwise stated.

5.3.2 Test gas(es)

The flammable gas(es) to be used in a mixture with clean air for initial and all subsequent tests shall be selected in accordance with a) to d) with decreasing priority.

- a) The specific gas for equipment intended for sensing a single flammable gas only.
- b) Methane for equipment intended for sensing methane or firedamp.
- c) Methane, and propane or butane for equipment intended for general purpose flammable gas detection (in order to get representative results, e.g. concerning sensitivity, response times and drift).
- d) A gas from the manufacturer's list of flammable gases for which the equipment is claimed to be suitable. The choice of this gas should be made by agreement between the manufacturer and the test laboratory.

For all the other gases for which the equipment is claimed to be suitable, the calibration curves and response times shall be supplied by the manufacturer and a representative sample verified by the testing laboratory. The tolerance on the nominal volume fraction of all test gases shall not exceed $\pm 10\%$. The volume fraction of the component within the test gas(es) shall be known to a relative expanded uncertainty of $\pm 2\%$ of the nominal value.

For the purpose of this standard, where it is appropriate to use zero gas rather than clean air, references to clean air may be regarded as references to zero gas.

The gas mixture may be prepared by any suitable method, for example in accordance with the methods outlined in ISO 6142 or ISO 6145, or by commercially produced certified gas mixtures.

5.3.3 Standard test gas

The volume fractions of the standard test gases shall be as follows:

- a) for Group I equipment indicating up to a volume fraction of 5 % methane: equivalent range of either a volume fraction of $(1,5 \pm 0,15)\%$ or a volume fraction of $(2,0 \pm 0,2)\%$, as agreed between the manufacturer and the testing laboratory;

- b) for other Group I and all Group II equipment: 45 % to 55 % of the measuring range, not within the explosive range wherever possible. If this concentration is within the explosive range, the flammable gas shall be mixed with nitrogen if the measuring function of the equipment is not affected by oxygen deficiency. Otherwise the volume fraction of the standard test gas shall be taken outside the explosive range as near as possible to the values stated above.

The volume fractions shall be known to a relative expanded uncertainty of not greater than ± 2 %.

5.3.4 Flow rate for test gases

When the equipment is exposed to the test gases, including air, the flow rate of the gas shall be in accordance with the instruction manual.

For equipment that samples by diffusion, either a calibration mask in accordance with 5.2.4 or a test chamber may be used.

5.3.5 Voltage

- a) Mains-powered and fixed DC powered equipment shall be operated within 2 % of the manufacturer's rated voltage and frequency.
- b) Battery-powered equipment shall, for short-term tests, be equipped with new or fully charged batteries at the commencement of each series of tests. For long-term testing, it is permissible to energize the unit from a stabilized power supply. The temperature test (5.4.6) shall be carried out with all batteries specified in the instruction manual.

5.3.6 Temperature

The ambient air and test gas shall be held at a temperature constant to ± 2 °C within the range of 15 °C to 25 °C, throughout the duration of each test, unless otherwise specified for the particular test. This requirement is not applicable to tests 5.4.12 and 5.4.21.

5.3.7 Pressure

The tests shall be performed at the prevailing ambient pressure provided that it lies between 86 kPa and 108 kPa. If a deviation greater than ± 1 kPa occurs during a test, the pressure changes shall be recorded and taken into account, using the results of the pressure test (5.4.7).

5.3.8 Humidity

The ambient air, zero gas and test gas shall be held at a relative humidity (RH) over the range 20 % to 80 % throughout each test unless otherwise specified for the particular test. The humidity of zero gas and test gas shall be controlled to within ± 10 % RH. This requirement is not applicable to tests 5.4.12 and 5.4.21.

For short applications of test gases (up to 8 hours), the use of dry gases is permitted. The properties of the measuring principle of the sensor shall be taken into account.

5.3.9 Acclimation time

In each instance where the equipment is subjected to a different test condition, the equipment shall be allowed to stabilize under these new conditions before measurements are taken.

5.3.10 Orientation

The equipment shall be tested in the orientation recommended by the manufacturer.

5.3.11 Communications options

For equipment that has serial or parallel communications options used during normal gas detection operation, tests in 5.4.3.2, 5.4.6 and 5.4.15 shall be performed with all communication ports connected. The maximum transaction rate, cabling characteristics and activity level specified by the instrument's manufacturer shall be employed.

5.3.12 Gas detection equipment as part of systems

For gas detection equipment that are part of systems, tests in 5.4.3.2, 5.4.6, 5.4.15 and 5.4.18 shall be performed with the maximum system communications transaction rate and activity level. This shall correspond to the largest and most complex system configuration permitted by the manufacturer.

5.4 Test methods

5.4.1 General

Tests shall be carried out, where applicable, to ensure that the equipment satisfies the construction requirements of 4.2. Most of the requirements for these tests are self-evident. For short-circuit requirements in 4.2.4, each wire connecting the equipment to any remote sensor or gas detection transmitter shall be substituted with a load resistor. The values of these resistors shall be equivalent to the maximum wire resistance for the cable specified in the instruction manual (see 4.4 d)). The device used for the short circuit shall be of negligible resistance and shall be applied at the remote sensor or gas detection transmitter ends of the load resistors.

The marking of the equipment and the contents of the instruction manual shall be confirmed against 4.3 and 4.4.

The following tests shall be performed in accordance with 5.3, unless otherwise stated. All tests shall be performed. At the end of each test, indications shall be taken in both clean air and the standard test gas, unless otherwise stated. The values of the indications used for verification of compliance with the performance requirements of Annex A shall be the final indications (see 3.6.2) of both the clean air and standard test gas readings, unless otherwise stated. If, however, the sensor characteristics do not allow the equipment to stabilize within 6 min, then a time shall be agreed between the manufacturer and the test laboratory when the equipment is deemed to be stabilized. This time shall not exceed 6 min and shall be specified in the instruction manual as the test gas application time for calibration. This time shall also be used for calibration and adjustment of the equipment, and when performing test 5.4.15.

For equipment having more than one selectable range for the same or different gases or vapours, each range shall be tested. For the second and subsequent ranges the necessary amount of testing shall be agreed upon between the manufacturer and the test laboratory.

For equipment where different ranges are achieved by using different sensors, each range shall be subjected to the full series of tests.

5.4.2 Unpowered storage

All parts of the equipment shall be exposed sequentially to the following conditions in clean air only:

- a) a temperature of (-25 ± 3) °C for at least 24 h;
- b) ambient temperature for at least 24 h;
- c) a temperature of (60 ± 2) °C for at least 24 h;
- d) ambient temperature for at least 24 h.

At each temperature, the humidity of the clean air shall be such that condensation does not occur.

5.4.3 Calibration and adjustment

5.4.3.1 Initial preparation of the equipment

The equipment shall be calibrated and adjustments shall be carried out to obtain correct indications in accordance with the manufacturer's instruction manual.

5.4.3.2 Calibration curve

The equipment shall be exposed to the gas selected in accordance with 5.3.2, at 0 %, 10 %, 30 %, 50 %, 70 % and 90 % of the measuring range, starting with the lowest and finishing with the highest of the selected volume fractions. However, the highest volume fraction may be reduced for equipment with low measuring ranges in order to prevent over-range indications within the performance limits.

This operation shall be carried out three times consecutively.

5.4.3.3 Response to different gases

For Group II equipment, the accuracies of the response curves or correction charts provided in the instruction manual shall be checked by measuring the response for the representative gases in accordance with 5.3.2, at a minimum of three different volume fractions spread evenly over the measuring range to verify response characteristics. This operation shall be carried out two times consecutively.

The ratio between the indication of the equipment (before correction using the manufacturer's response curve or correction charts) and the gas volume fraction obtained for each of the three gas volume fractions of each gas tested shall not be less than 0,4 and shall not exceed 2,0.

Equipment with semiconductor or catalytic sensors shall then be exposed to the test gas with a volume fraction between 45 % to 55 % of the measuring range for (60 +2/0) min and the deviation of the indication during the exposure measured.

5.4.4 Stability

5.4.4.1 Battery-powered equipment for stability

For these tests, battery-powered equipment should be powered from internal batteries wherever possible, otherwise an external power supply may be used.

5.4.4.2 Short-term stability

The equipment shall be exposed to six applications of the standard test gas for 3 min followed by exposure to clean air for a period of 7 min. Indications shall be taken at the end of each exposure to clean air and the standard test gas.

5.4.4.3 Long-term stability (fixed and transportable equipment – Group I only)

The equipment shall be operated in clean air continuously for a period of (28 +1/0) days and shall be exposed to the standard test gas for an (480 +10/0) min period at (7 ± 1) day intervals over the test period. Indications shall be taken prior to the application of, after stabilization and prior to removal of the standard test gas.

After this first period, the following procedure shall be performed.

The equipment shall be exposed to a methane-air mixture with a volume fraction of 1,0 % (v/v) \pm 0,05 % (v/v) for (168 \pm 4) hours, a minimum of 5 indications being taken no less than 24 hours apart in clean air and the standard test gas. One of these indications shall be taken at the beginning of the test and another at the end of the test.

5.4.4.4 Long-term stability (portable equipment – Group I only)

The equipment shall be operated in clean air continuously for a period of (490 \pm 10/0) min per working day over a total of 20 consecutive working days. The equipment shall be exposed to the standard test gas for (60 \pm 2) min during each operating period. Indications shall be taken prior to the application of, after stabilization, and prior to removal of the standard test gas.

After this first period, the following procedure shall be performed starting at the next working day.

The equipment shall be operated in a methane-air mixture with a volume fraction of 1,0 % (v/v) \pm 0,05 % (v/v) for (480 \pm 2) min, taking indications in clean air and the standard test gas at the end of this period. The equipment shall then be switched off and exposed to clean air over night. This cycle shall be repeated for a further 4 consecutive working days.

5.4.4.5 Long-term stability (fixed and transportable equipment – Group II only)

The equipment shall be operated continuously in clean air for a period of (63 \pm 1) days. On the eighth day, the equipment shall be exposed to the standard test gas for a (480 \pm 10/0) min period. Indications shall be taken prior to the application of test gas, after stabilization of the reading and prior to the removal of test gas.

At the end of each subsequent (7 \pm 1) day period, the equipment shall be exposed to the standard test gas until the reading has stabilized. Indications shall be taken prior to the application of test gas and after stabilization of the reading.

5.4.4.6 Long-term stability (portable equipment – Group II only)

The equipment shall be operated continuously in clean air for a period of (420 \pm 5/0) min and then exposed to the standard test gas for another (60 \pm 5/0) min. Indications shall be taken prior to the application of test gas, after stabilization of the reading and prior to removal of test gas.

The equipment shall then be operated in clean air continuously for a period of (480 \pm 10/0) min per working day over a total of 19 consecutive working days. The equipment shall be exposed to the standard test gas until the reading has stabilized, once at the end during each operating period. Indications shall be taken prior to the application of test gas and after stabilization of the reading.

5.4.5 Alarm set point(s)

5.4.5.1 Rising concentration

For equipment with adjustable alarm set points, set the alarm set point at 10 % relative below the concentration of the standard test gas.

If the alarm set point cannot be set at this concentration, the alarm shall be set as near as possible to that concentration. In this case and for equipment with fixed alarm set points the test gas shall have a volume fraction of 10 % relative above the concentration of the alarm set point.

The equipment shall be adjusted with clean air and standard test gas or the specified test gas. Then expose the equipment to clean air and then to the standard test gas or the specified test gas until alarm activation or twice the respective $t(90)$, whichever is less.

For equipment with several alarm set points, this test shall be carried out for each alarm set point.

5.4.5.2 Falling concentration (for equipment with measuring range over UFL only)

For equipment with adjustable alarm set points, set the alarm set point at UFL plus 10 % of the measuring range. If the alarm set point cannot be set at this concentration, the alarm shall be set as near as possible to that concentration.

The specified test gas shall have a volume fraction of the alarm set point minus 5 % of the measuring range.

The equipment shall be adjusted with standard test gas and clean air or the specified test gas. Then expose the equipment to a test gas with a volume fraction of 90 % of the measuring range and then to the specified test gas until alarm activation or twice the respective $t(90)$, whichever is less.

For equipment with several alarm set points, this test shall be carried out for each alarm set point.

5.4.6 Temperature

This test shall be performed in a temperature chamber having the capability of holding the remote sensor or equipment at the specified temperature within ± 2 °C. The remote sensor or equipment shall be acclimated at each temperature specified in Annex A, as appropriate, for at least 3 h or until acclimated within ± 2 °C for a minimum of 1 h. The remote sensor or equipment shall be exposed sequentially to clean air and the standard test gas, which shall be at the same temperature as the atmosphere in the test chamber. The dew point of the air or standard test gas shall be below the lowest temperature of the test chamber.

For battery powered equipment, the test shall be carried out with all batteries specified in the instruction manual.

5.4.7 Pressure

The effects of pressure variation shall be observed by placing the remote sensor or equipment (including the aspirator for aspirated equipment) in a test chamber that permits the pressure of clean air and of the standard test gas to be varied over the range specified in Annex A.

The pressure shall be maintained at the specified levels within $\pm 0,5$ kPa for 5 min, before a reading is accepted or a test is made. Readings shall be taken with clean air and standard test gas.

5.4.8 Humidity of test gas

The test shall be conducted at temperature of (40 ± 2) °C. After an acclimation time of at least 2 hours at 40 °C, the equipment shall be calibrated and adjusted in accordance with the instruction manual (see 4.4 b) and 4.4 d)13)). The sensor shall be exposed for $(60 +5/0)$ min to clean air humidified to (20 ± 5) % RH. The sensor shall then be exposed to the standard test gas humidified to (20 ± 5) % RH until stabilized. The procedure shall be repeated with humidities of (50 ± 5) % RH and (90 ± 5) % RH. The concentration of the test gas shall be held constant, or due allowance of changes in its concentration by dilution in water shall be made.

All relative humidity shall be considered as water vapour volume fractions at the nominal temperature of 40 °C.

5.4.9 Air velocity

This test is applicable to diffusion equipment only.

The equipment or the remote sensor shall be tested in a flow chamber in both clean air and standard test gas.

For equipment with integral sensors, which are too large to be tested in a flow chamber, other flow equipment for carrying out the test shall be permitted. In this case the "other flow equipment" shall be described in the test report.

The sensor shall be operated in the orientation recommended by the manufacturer. If there is no such recommendation e.g. for portable equipment, a typical orientation shall be used.

Irrespective of whether a flow chamber or other flow equipment is used, the direction of the air flow with respect to the sensor inlet shall be as follows:

- 1) flow directed at the sensor inlet;
- 2) flow directed 180° to 1);
- 3) flow directed 90° to 1).

Each orientation is given with a tolerance of $\pm 5^\circ$.

Measurements shall be made under:

- non-forced ventilation conditions
- at $(3 \pm 0,3)$ m/s and
- at $(6 \pm 0,6)$ m/s.

Directions of flow which are prohibited within the instruction manual shall not be tested.

5.4.10 Flow rate for aspirated equipment

The equipment shall be tested by varying the flow rate in both clean air and standard test gas

- 1) from the nominal flow rate to 130 % of the nominal flow rate, if possible
- 2) from the nominal flow rate to 110 % of the flow rate at which the flow failure signal is activated, or to 50 % of the nominal flow rate if a flow failure signal is not provided.

5.4.11 Orientation

5.4.11.1 Portable equipment

During tests with clean air and standard test gas, rotate the sensor, or the whole equipment if relevant, through 360° in steps of 90° around each of its three mutually perpendicular axes (one axis at a time). Record the indication in each position.

5.4.11.2 Fixed and transportable equipment

Test the equipment or remote sensor with clean air and standard test gas within the orientation limits stated in the manufacturer's instructions, but in no case less than a deviation of $\pm 15^\circ$ from the nominal orientation.

5.4.12 Vibration

5.4.12.1 Test equipment

The vibration test machine shall consist of a vibrating table capable of producing a vibration of variable frequency and amplitude with the test equipment mounted in place, as required by EN 60068-2-6 and the following test procedures.

5.4.12.2 Procedures

5.4.12.2.1 General

The test shall be carried out in accordance with EN 60068-2-6.

The equipment shall be energized and mounted on the vibration test machine and vibrated successively in each of three planes respectively parallel to each of the three major axes of the equipment.

An adjustable alarm set point shall be set to 20 % of measuring range.

Before, and at the conclusion of the test, the equipment shall be exposed to clean air followed by the standard test gas.

The equipment shall be mounted on the vibration table in the same manner as intended for use including any resilient mounts, carrier or holding devices that are provided as standard parts of the equipment.

The equipment shall be vibrated over the frequency range specified at the excursion or constant acceleration peak specified, for a period of at least 1 h in each of the three mutually perpendicular planes. The frequency shall continuously change exponentially with time and the rate of change of frequency shall be one octave per minute.

5.4.12.2.2 Procedure 1

For remote sensors and all equipment with integral sensors, the vibration shall be as follows:

- 10 Hz to 31,5 Hz, 0,5 mm displacement amplitude (1,0 mm peak-peak total excursion)
- 31,5 Hz to 150 Hz, 19,6 m/s² acceleration amplitude

5.4.12.2.3 Procedure 2

For all other equipment, the vibration shall be as follows:

- 10 Hz to 31,5 Hz, 0,5 mm displacement amplitude (1,0 mm peak-peak total excursion)
- 31,5 Hz to 100 Hz, 19,6 m/s² acceleration amplitude

5.4.13 Drop test for portable and transportable equipment

If the manufacturer recommends that the instrument be used in its protective casing, the test shall be carried out with the protective casing installed.

If components of fixed equipment can be used like portable or transportable equipment according to the instruction manual, these components should be considered to be portable or transportable for this test.

Before, and at the conclusion of the test, the equipment shall be exposed to clean air followed by the standard test gas.

Portable equipment shall be released, while operating, from a height of $(1 +0,05/0)$ m above a concrete surface and allowed to free fall.

Transportable equipment with a mass less than 5 kg shall be released, while not operating, from a height of $(0,3 +0,03/0)$ m above a concrete surface and allowed to free fall.

Other transportable equipment shall be released, while not operating, from a height of $(0,1 +0,02/0)$ m above a concrete surface and allowed to free fall.

All heights are measured from the lowest point of the equipment.

The test required above shall be performed three separate times, the portable equipment being released each time with a different side (surface) facing down at the time of release and the transportable equipment to be in an orientation for normal transport.

The equipment shall be considered to have failed this test if there is a loss of function (e.g. alarm, pump function, controls, display) after the test.

Automatic re-starting or shut-down of the equipment shall not occur during the test.

5.4.14 Warm-up time

An adjustable alarm set point shall be set to 20 % of the measuring range.

The equipment shall be switched off and left for at least 24 h in clean air. After the 24 h period, the equipment shall be switched on in clean air and the warm-up time measured.

Group I equipment shall be switched off for a further 24 h in clean air. After this period, the equipment shall be exposed for $(5 +0,5/0)$ min to the standard test gas, then switched on in the presence of the test gas and the warm-up time measured.

Where equipment prompts the user to perform any adjustment during start-up, the test shall be applied for the 'Yes' and 'No' options.

5.4.15 Time of response

The equipment shall be switched on in clean air and, after an interval corresponding to at least two times the warm-up time, as determined in accordance with 5.4.14, without switching off, the equipment or the sensor(s) shall be subjected to step changes from clean air to the standard test gas and from standard test gas to clean air. These changes shall be introduced by means of suitable equipment (see Annex B).

The times of response $t(50)$ and $t(90)$ for increasing concentration, and $t(50)$ and $t(10)$ for decreasing concentration shall be measured.

For an optional sampling probe, an extra test is required to measure the additional delay. This shall be less than 3 s/m of the total length of the probe plus tubing or any greater value, which is stated in the instruction manual.

5.4.16 High gas concentration operation above the measuring range

This subclause applies to all equipment with an upper limit of the measuring range less than 100 % (v/v) gas.

The sensor shall be subjected to the test using test equipment that simulates a step change between gas concentrations such as those described in Annex B.

The sensor shall be subjected to a step change from clean air to a volume fraction of 100 % (v/v) gas that shall be maintained for (180 +5/0) s. The equipment or remote sensor shall then be subjected to clean air for (20 +2/0) min, followed by the standard test gas.

All gas concentrations above full scale shall be indicated by a full scale indication and, where fitted, an alarm. If the indication is digital, a clear indication shall be given that the upper limit of the measuring range has been exceeded.

All gas alarms shall remain in operation at all gas concentrations above full scale. If the equipment provides a latching alarm feature, the latching feature shall be verified during and after application of the high gas concentration.

5.4.17 Battery capacity

5.4.17.1 Battery discharge

With a battery fully charged at the beginning of the test, the equipment shall be operated at maximum load condition with consideration to quantity and type of sensors in clean air for a total period of

- a) (480 +5/0) min, if fitted with a user-operable on/off switch;
- b) (600 +5/0) min, if not so fitted; or
- c) any longer time as specified by the manufacturer.

At the beginning and end of the specified period, the equipment is exposed to clean air and the standard test gas.

5.4.17.2 Low battery duration

The equipment shall then continue to operate until an indication that the low battery condition has been reached. The equipment shall continue to operate for at least an additional (10 +0,5/0) min and then be exposed to the standard test gas.

Where it is impractical to discharge the equipment continuously, the equipment may be switched off (e.g. overnight) to ensure the low battery condition is observed in the required time.

5.4.18 Power supply variations

The equipment shall be set up under normal conditions (see 5.3), at rated voltage and, where appropriate, rated frequency. For equipment with remote sensors, the test shall be performed with both maximum and minimum resistance of the interconnecting cable. The equipment shall then be subjected to the following tests.

The equipment calibration shall be checked at both 115 % and 80 % of rated voltage and at +2 % above the minimum supply voltage fault limit.

Where the manufacturer of the equipment specifies a supply range other than those specified above, the equipment shall be tested at the upper and lower limits of the supply voltage specified by the manufacturer.

It shall be verified at +2 % above the minimum supply voltage fault limit that all output functions are working properly even at the worst case load conditions.

Analogue outputs shall be tested at the maximum output level. Relays shall be able to energize at +2 % above the minimum supply voltage fault limit.

5.4.19 Addition of sampling probe

When it is intended to add a sampling probe, the equipment shall first be calibrated using clean air and the standard test gas without the sampling probe. The sampling probe shall then be added, and clean air and standard test gas applied again.

5.4.20 Other gases and poisons

5.4.20.1 Other gases

The equipment shall be tested separately with the following gas mixtures:

- a) Group I equipment indicating up to a volume fraction of 5 % methane in air:
 - 1) a methane volume fraction of the standard test gas + a volume fraction of 13 % oxygen in nitrogen;
 - 2) a methane volume fraction of the standard test gas + a volume fraction of 5 % carbon dioxide in air;
 - 3) a methane volume fraction of the standard test gas + a volume fraction of 0,075 % ethane in air.
- b) Group I equipment indicating up to a volume fraction of 100 % methane in air:
 - 1) a volume fraction of 50 % methane + a volume fraction of 6,5 % oxygen in nitrogen;
 - 2) a volume fraction of 50 % methane + a volume fraction of 5 % carbon dioxide in nitrogen;
 - 3) a volume fraction of 50 % methane + a volume fraction of 2,5 % ethane in nitrogen.

The gas mixtures may be prepared by any suitable method. The tolerances on the volume fraction of each component shall be within ± 10 % of its nominal concentration.

The volume fraction of each component shall be known to a relative expanded uncertainty of ± 2 % of the stated value.

5.4.20.2 Poisons (applicable only to Group I equipment with catalytic or semiconductor sensors)

The equipment shall be exposed to a volume fraction of $(1,0 \pm 0,05)$ % methane in air mixture containing a volume fraction of (10 ± 1) ppm of hexamethyldisiloxane and shall perform in continuous operation until a dose of (400 ± 20) ppm min is reached.

NOTE 1 Certain materials that might be present in industrial atmospheres can lead to "poisoning" or other undesirable effects which can result in a change of sensitivity of a gas sensor.

NOTE 2 As improved tolerances to these materials are frequently claimed by manufacturers, evidence of the testing procedure used to substantiate these claims and test results can be open to validation or verification by agreement between a purchaser, a manufacturer, and a testing laboratory. Possible "poisoning" agents and their effects on sensor performance are discussed in IEC EN 60079-29-2 IEC.

NOTE 3 The time the equipment is exposed is calculated by dividing the required dose by the actual concentration of hexamethyldisiloxane.

IEC 5.4.21 Electromagnetic compatibility

The equipment shall be set up under normal conditions, in accordance with 5.3, and then shall be subjected to the tests specified in EN 50270. IEC

5.4.22 Field calibration kit

Calibration initiation methods and gas application methods shall be tested or excluded from the scope of the performance test within the instruction manual.

Field calibration kit(s) shall be verified by comparison of the following:

- a) expose the equipment to clean air and standard test gas using the field calibration kit in accordance with the instruction manual;
- b) expose the equipment to clean air and standard test gas as it is done in normal operation.

5.4.23 Verification of software and digital components

Design and function of the equipment using software and/or digital technologies shall be evaluated and tested in accordance with EN 50271.

<http://www.china-gauges.com/>

Annex A (normative)

Performance requirements

Table A.1 – Performance requirements (1 of 6)

NOTE The specified numbers are the maximum permitted deviations of the indications of the equipment from the reference indications obtained at the start of the test or at reference conditions (e.g. at reference temperature 20 °C).

Sub-clause	Test	Group I equipment limits (whichever value is greater)		Group II equipment limits (whichever value is greater)		
		Volume fraction up to 5 % methane in air	Volume fraction up to 100 % methane in air	Volume fraction up to 20 % lower flammable limit	Volume fraction up to 100 % lower flammable limit	Volume fraction up to 100 % gas
5.4.2	Unpowered storage	None	None	None	None	None
5.4.3.2	Calibration curve	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication
5.4.3.3	Response to different gases	Not applicable	Not applicable	±7 % measuring range or ±15 % of indication	±7 % measuring range or ±15 % of indication	±7 % measuring range or ±15 % of indication
5.4.4.2	Stability, short term	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±3 % measuring range or ±10 % of indication	±3 % measuring range or ±10 % of indication	±3 % measuring range or ±10 % of indication
5.4.4.3 and 5.4.4.5	Stability, long term (fixed/transportable)	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±15 % measuring range or ±30 % of indication	±7 % measuring range or ±20 % of indication	±7 % measuring range or ±20 % of indication
5.4.4.4 and 5.4.4.6	Stability, long term (portable)	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±10 % measuring range or ±20 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication
5.4.5	Alarm set point(s)	Check alarm/manual reset operation	Check alarm/manual reset operation	Check alarm/manual reset operation	Check alarm/manual reset operation	Check alarm/manual reset operation
5.4.6 (a)	Temperature (portable)	±0,3 % methane or ±15 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)	±5 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)	±10 % measuring range or ±20 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)	±5 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)	±5 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)

www.china-gauges.com/

Table A.1 (2 of 6)

Sub-clause	Test	Group I equipment limits (whichever value is greater)		Group II equipment limits (whichever value is greater)		
		Volume fraction up to 5 % methane in air	Volume fraction up to 100 % methane in air	Volume fraction up to 20 % lower flammable limit	Volume fraction up to 100 % lower flammable limit	Volume fraction up to 100 % gas
5.4.6 (b)	Temperature (non-portable equipment including remote sensors with restricted temperature range)	Not applicable	Not applicable	Control unit: ±3 % measuring range or ±10 % of indication from 20 °C (test: 5 °C, 20 °C, 55 °C) All other equipment: ±10 % measuring range or ±30 % of indication from 20 °C (test: 5 °C, 20 °C, 55 °C)	Control unit: ±3 % measuring range or ±10 % of indication from 20 °C (test: 5 °C, 20 °C, 55 °C) All other equipment: ±5 % measuring range or ±15 % of indication from 20 °C (test: 5 °C, 20 °C, 55 °C)	Control unit: ±3 % measuring range or ±10 % of indication from 20 °C (test: 5 °C, 20 °C, 55 °C) All other equipment: ±10 % measuring range or ±20 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C)
5.4.6 (c)	Temperature (all other non- portable equipment including remote sensors)	±0,3 % methane or ±15 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)	±5 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 40 °C)	Control unit: ±3 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C) All other equipment: ±20 % measuring range or ±40 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C)	Control unit: ±3 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C) All other equipment: ±10 % measuring range or ±20 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C)	Control unit: ±3 % measuring range or ±10 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C) All other equipment: ±10 % measuring range or ±20 % of indication from 20 °C (test: -20 °C, 20 °C, 55 °C)

<http://www.china-gauges.com/>

Table A.1 (3 of 6)

Sub-clause	Test	Group I equipment limits (whichever value is greater)		Group II equipment limits (whichever value is greater)		
		Volume fraction up to 5 % methane in air indication	Volume fraction up to 100 % methane in air indication	Volume fraction up to 20 % lower flammable limit indication	Volume fraction up to 100 % lower flammable limit indication	Volume fraction up to 100 % gas indication
5.4.7	Pressure	±0,2 % methane or ±30 % of indication from 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)	±5 % measuring range or ±30 % of indication from 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)	±10 % measuring range or ±30 % of indication from 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)	±5 % measuring range or ±30 % of indication from 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)	±5 % measuring range or ±30 % of indication from 100 kPa (test: 80 kPa, 100 kPa, 120 kPa)
5.4.8	Humidity of test gas	±0,2 % methane or ±15 % of indication from the indication at adjustment at 40 °C (test: 20 %RH, 50 %RH, 90 %RH)	±5 % measuring range or ±15 % of indication from the indication at adjustment at 40 °C (test: 20 %RH, 50 %RH, 90 %RH)	±15 % measuring range or ±30 % of indication from the indication at adjustment at 40 °C (test: 20 %RH, 50 %RH, 90 %RH)	±10 % measuring range or ±30 % of indication from the indication at adjustment at 40 °C (test: 20 %RH, 50 %RH, 90 %RH)	±10 % measuring range or ±30 % of indication from the indication at adjustment at 40 °C (test: 20 %RH, 50 %RH, 90 %RH)
5.4.9	Air velocity	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±10 % measuring range or ±20 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication
5.4.10	Flow rate	±0,1 % methane or ±5 % of indication from that at nominal flow rate	±3 % measuring range or ±5 % of indication from that at nominal flow rate	±10 % measuring range or ±20 % of indication from that at nominal flow rate	±5 % measuring range or ±10 % of indication from that at nominal flow rate	±5 % measuring range or ±10 % of indication from that at nominal flow rate

www.china-gauges.com/

Table A.1 (4 of 6)

Sub-clause	Test	Group I equipment limits (whichever value is greater)		Group II equipment limits (whichever value is greater)		
		Volume fraction up to 5 % methane in air indication	Volume fraction up to 100 % methane in air indication	Volume fraction up to 20 % lower flammable limit indication	Volume fraction up to 100 % lower flammable limit indication	Volume fraction up to 100 % gas indication
5.4.11	Orientation	±0,1 % methane or ±5 % of indication	Portable: ±5 % measuring range or ±10 % of indication Fixed/transportable: ±3 % measuring range or ±5 % of indication	±10 % measuring range or ±20 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication
5.4.12	Vibration	±0,1 % methane or ±5 % of indication, and no loss of function, no fault signal, no damage resulting in a hazard and no false alarms	±3 % measuring range or ±5 % of indication, and no loss of function, no fault signal, no damage resulting in a hazard and no false alarms	±10 % measuring range or ±20 % of indication, and no loss of function, no fault signal, no damage resulting in a hazard and no false alarms	±5 % measuring range or ±10 % of indication, and no loss of function, no fault signal, no damage resulting in a hazard and no false alarms	±5 % measuring range or ±10 % of indication, and no loss of function, no fault signal, no damage resulting in a hazard and no false alarms
5.4.13	Drop test	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±10 % measuring range or ±20 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication
5.4.14	Warm-up time	Fixed/transportable: ±0,1 % methane within 5 min, and no false alarm Portable: ±0,1 % methane within 2 min, and no false alarm	Fixed/transportable: ±3 % measuring range within 5 min, and no false alarm Portable: ±3 % measuring range within 2 min, and no false alarm	Fixed/transportable: ±5 % measuring range within manual spec., and no false alarm Portable: ±5 % measuring range within 2 min, and no false alarm	Fixed/transportable: ±5 % measuring range within manual spec., and no false alarm Portable: ±5 % measuring range within 2 min, and no false alarm	Fixed/transportable: ±5 % measuring range within manual spec., and no false alarm Portable: ±5 % measuring range within 2 min, and no false alarm
5.4.15	Time of response (increasing concentration)	t(50) in less than 10 s t(90) in less than 30 s	t(50) in less than 10 s t(90) in less than 30 s	t(50) in less than 20 s t(90) in less than 60 s	t(50) in less than 20 s t(90) in less than 60 s	t(50) in less than 20 s t(90) in less than 60 s
5.4.15	Time of response (decreasing concentration)	t(50) in less than 30 s t(10) in less than 90 s	t(50) in less than 10 s t(10) in less than 30 s	Not applicable	Not applicable	t(50) in less than 20 s t(10) in less than 60 s

Table A.1 (5 of 6)

Sub-clause	Test	Group I equipment limits (whichever value is greater)		Group II equipment limits (whichever value is greater)		
		Volume fraction up to 5 % methane in air indication	Volume fraction up to 100 % methane in air indication	Volume fraction up to 20 % lower flammable limit indication	Volume fraction up to 100 % lower flammable limit indication	Volume fraction up to 100 % gas indication
5.4.16	High gas concentration operation above the measuring range	$\pm 0,2$ % methane or $+20$ % / -10 % of indication	± 5 % measuring range or ± 10 % of indication	Fault indication after reset or ± 15 % measuring range or $+40$ % / -20 % of indication	Fault indication after reset or ± 7 % measuring range or $+20$ % / -10 % of indication	± 7 % measuring range or ± 15 % of indication
5.4.17	Battery capacity	$\pm 0,1$ % methane or ± 5 % of indication (test: 8 h or 10 h, respectively) $\pm 0,2$ % methane or ± 10 % of indication (test: 10 min after "low battery" condition)	± 3 % measuring range or ± 5 % of indication (test: 8 h or 10 h, respectively) ± 6 % measuring range or ± 10 % of indication (test: 10 min after "low battery" condition)	± 7 % measuring range or ± 15 % of indication (test: 8 h or 10 h, respectively) or ± 10 % measuring range or ± 20 % of indication (test: 10 min after "low battery" condition)	± 5 % measuring range or ± 10 % of indication (test: 8 h or 10 h, respectively) or ± 7 % measuring range or ± 15 % of indication (test: 10 min after "low battery" condition)	± 3 % measuring range or ± 10 % of indication (test: 8 h or 10 h, respectively) or ± 6 % measuring range or ± 20 % of indication (test: 10 min after "low battery" condition)
5.4.18	Power supply variation	$\pm 0,1$ % methane or ± 5 % of indication from that at rated voltage.	± 3 % measuring range or ± 5 % of indication from that at rated voltage.	± 5 % measuring range or ± 10 % of indication from that at rated voltage.	± 5 % measuring range or ± 10 % of indication from that at rated voltage.	± 3 % measuring range or ± 10 % of indication from that at rated voltage.
5.4.19	Addition of sampling probe	$\pm 0,1$ % methane or ± 5 % of indication	± 3 % measuring range or ± 5 % of indication	± 5 % measuring range or ± 10 % of indication	± 5 % measuring range or ± 10 % of indication	± 5 % measuring range or ± 10 % of indication

http://www.china-gauges.com/

Table A.1 (6 of 6)

Sub-clause	Test	Group I equipment limits (whichever value is greater)		Group II equipment limits (whichever value is greater)		
		Volume fraction up to 5 % methane in air indication	Volume fraction up to 100 % methane in air indication	Volume fraction up to 20 % lower flammable limit indication	Volume fraction up to 100 % lower flammable limit indication	Volume fraction up to 100 % gas indication
5.4.20.1	Other gases	±10 % of the actual methane volume fraction applied	±10 % of the actual methane volume fraction applied	Not applicable	Not applicable	Not applicable
5.4.20.2	Poisons	±0,2 % methane or ±10 % of indication	±3 % measuring range or ±10 % of indication	Not applicable	Not applicable	Not applicable
5.4.21	Electromagnetic compatibility	According to EN 50270	According to EN 50270	According to EN 50270	According to EN 50270	According to EN 50270
5.4.22	Field calibration kit	±0,1 % methane or ±5 % of indication	±3 % measuring range or ±5 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication	±5 % measuring range or ±10 % of indication

<http://www.china-gauges.com/>

Annex B (informative)

Determination of time of response

B.1 Aspirated equipment

B.1.1 Test rig

Attach the equipment to the test rig as shown schematically in Figure B.1.

The test rig consists of two gas lines, one supplying clean air and the other test gas. The two flows can be switched between the equipment inlet and the exhaust. While one flow is directed to the equipment, the other flow is directed to the exhaust. Switching of the two flows should be done simultaneously.

The gas line connecting the test rig to the equipment should have an outlet for excess gas.

The volume of the gas line connecting the test rig to the equipment should be kept to a minimum.

B.1.2 Equipment without internal pump

The outlet for excess gas should be closed.

The flow rates of the two gas lines should be set to the minimum flow rate specified in the instruction manual.

The measurement of the time of response should start with the switching from clean air to test gas. Where appropriate, a correction should be made to the time of response for the switching time between the two gas lines and for the time needed to purge the dead volume between the outlet of the switching device and the equipment inlet.


B.1.3 Equipment with internal pump

The outlet for excess gas should be opened.

The gas inlet to the equipment should be appropriately restricted so that the flow rate to the equipment is 10 % above the flow rate at which the flow failure signal is activated.

The flow rates of the two gas lines should be set appropriately. The excess flow rate at the outlet should be sufficiently high so that reverse flow cannot occur. This will usually be achieved by an excess flow rate of approximately 20 %.

The measurement of the time of response should start with the switching from clean air to test gas. Where appropriate, a correction should be made to the time of response for the switching time between the two gas lines and for the time needed to purge the dead volume between the outlet of the switching device and the equipment inlet.

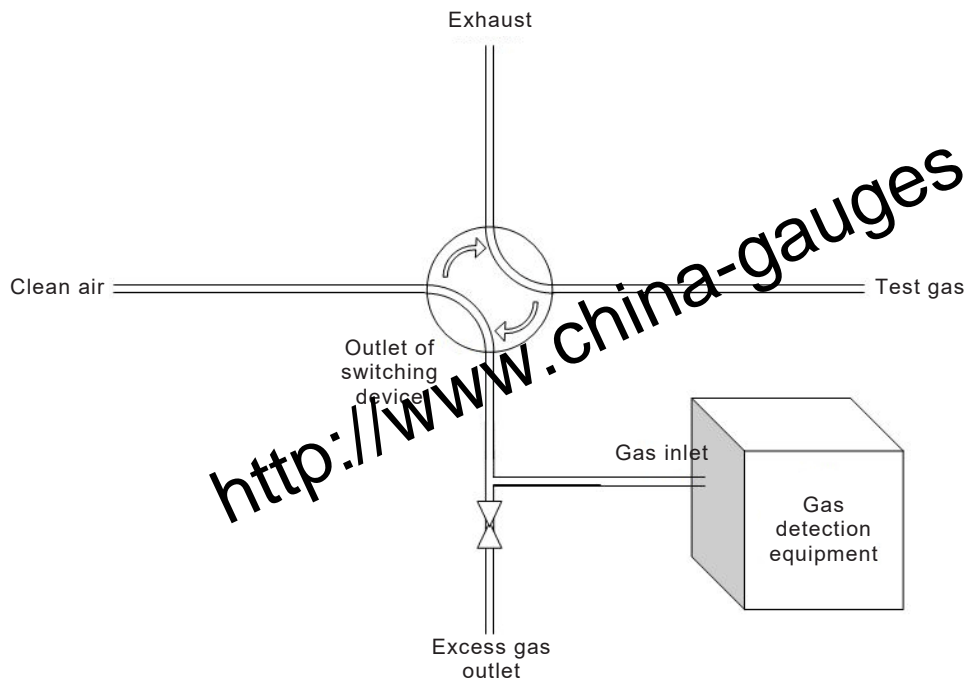

IEC

Figure B.1 – Schematic example of test rig for use with aspirated equipment

B.2 Equipment that samples by diffusion

B.2.1 Calibration mask method

This method should only be used for measuring response times of "other gases" (5.3.2) in order to compare the response times of different gases.

The test rig described in B.1.1 should be used. The test should be performed as for equipment without an internal pump (see B.1.2).

The flow rate through the mask should be set to the minimum flow rate specified in the instruction manual. If only a nominal flow rate is given, this nominal flow rate should be used.

B.2.2 Diffusion or flow methods

The diffusion and/or flow method should be used for measuring the time of response of the equipment for the standard test gases according to 5.4.15.

A suitable method should be used which has been validated. Examples are diffusion (by immersion or containment) or flow methods.

Bibliography

IEC 60050, *International Electrotechnical Vocabulary (IEV)*

IEC 60529, *Degrees of protection provided by enclosures (IP Code)*

☐ NOTE Harmonized as EN 60529. ☐

IEC 60079-1, *Explosive atmospheres – Part 1: Equipment protection by flameproof enclosures “d”*

☐ NOTE Harmonized as EN 60079-1. ☐

IEC 60079-2, *Explosive atmospheres – Part 2: Equipment protection by pressurized enclosure “p”*

☐ NOTE Harmonized as EN 60079-2. ☐

IEC 60079-5, *Explosive atmospheres – Part 5: Equipment protection by powder filling “q”*

☐ NOTE Harmonized as EN 60079-5. ☐

IEC 60079-6, *Explosive atmospheres – Part 6: Equipment protection by liquid immersion “o”*

☐ NOTE Harmonized as EN 60079-6. ☐

IEC 60079-7, *Explosive atmospheres – Part 7: Equipment protection by increased safety “e”*

☐ NOTE Harmonized as EN 60079-7. ☐

IEC 60079-10-1, *Explosive atmospheres – Part 10-1: Classification of areas – Explosive gas atmospheres*

☐ NOTE Harmonized as EN 60079-10-1. ☐

IEC 60079-11, *Explosive atmospheres – Part 11: Equipment protection by intrinsic safety “i”*

☐ NOTE Harmonized as EN 60079-11. ☐

IEC 60079-15, *Explosive atmospheres – Part 15: Equipment protection by type of protection “n”*

☐ NOTE Harmonized as EN 60079-15. ☐

IEC 60079-18, *Explosive atmospheres – Part 18: Equipment protection by encapsulation “m”*

☐ NOTE Harmonized as EN 60079-18. ☐

IEC 60079-25, *Explosive atmospheres – Part 25: Intrinsically safe electrical systems*

☐ NOTE Harmonized as EN 60079-25. ☐

IEC 60079-26, *Explosive atmospheres – Part 26: Equipment with equipment protection level (EPL) Ga*

☐ NOTE Harmonized as EN 60079-26. ☐

IEC 60079-29-2, *Explosive atmospheres – Part 29-2: Gas detectors – Selection, installation, use and maintenance of detectors for flammable gases and oxygen*

☐ NOTE Harmonized as EN 60079-29-2. ☐

<http://www.china-gauges.com/>

IEC 60079-29-3, *Explosive atmospheres – Part 29-3: Gas detectors – Guidance on functional safety of fixed gas detection systems*

NOTE Harmonized as EN 60079-29-3.

IEC 60079-29-4, *Explosive atmospheres – Part 29-4: Gas detectors – Performance requirements of open path detectors for flammable gases*

NOTE Harmonized as EN 60079-29-4.

ISO 6142, *Gas analysis – Preparation of calibration gas mixtures – Gravimetric method*

NOTE Harmonized as EN ISO 6142²⁾.

ISO 6145-1, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 1: Methods of calibration*

NOTE Harmonized as EN ISO 6145-1.

ISO 6145-2, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 2: Volumetric pumps*

ISO 6145-4, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 4: Continuous syringe injection method*

NOTE Harmonized as EN ISO 6145-4.

ISO 6145-5, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 5: Capillary calibration devices*

NOTE Harmonized as EN ISO 6145-5.

ISO 6145-6, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 6: Critical orifices*

NOTE Harmonized as EN ISO 6145-6.

ISO 6145-7, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 7: Thermal mass-flow controllers*

NOTE Harmonized as EN ISO 6145-7.

ISO 6145-9, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 9: Saturation method*

NOTE Harmonized as EN ISO 6145-9.

ISO 6145-10, *Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 10: Permeation method*

NOTE Harmonized as EN ISO 6145-10.

²⁾ Superseded by EN ISO 6142-1 (ISO 6142-1).

<http://www.china-gauges.com/>

<http://www.china-gauges.com/>

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Copyright in BSI publications

All the content in BSI publications, including British Standards, is the property of and copyrighted by BSI or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use.

Save for the provisions below, you may not transfer, share or disseminate any portion of the standard to any other person. You may not adapt, distribute, commercially exploit, or publicly display the standard or any portion thereof in any manner whatsoever without BSI's prior written consent.

Storing and using standards

Standards purchased in soft copy format:

- A British Standard purchased in soft copy format is licensed to a sole named user for personal or internal company use only.
- The standard may be stored on more than 1 device provided that it is accessible by the sole named user only and that only 1 copy is accessed at any one time.
- A single paper copy may be printed for personal or internal company use only.

Standards purchased in hard copy format:

- A British Standard purchased in hard copy format is for personal or internal company use only.
- It may not be further reproduced – in any format – to create an additional copy. This includes scanning of the document.

If you need more than 1 copy of the document, or if you wish to share the document on an internal network, you can save money by choosing a subscription product (see 'Subscriptions').

Reproducing extracts

For permission to reproduce content from BSI publications contact the BSI Copyright & Licensing team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email subscriptions@bsigroup.com.

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Useful Contacts

Customer Services

Tel: +44 345 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 345 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK